# HIOKI

CM4141 CM4142

**AC CLAMP METER** 

Instruction Manual



EN

Jan. 2021 Revised edition 3 CM4141A961-03 21-01H



# **Operating Precautions**

# **MWARNING**

Your instrument can be used to measure voltages in excess of 1000 V DC if and only if both of the following conditions are satisfied:

- The circuit under measurement is isolated from the commercial power grid.
- 2. The circuit under measurement is isolated from ground.
- e.g.: when measuring the no-load voltage of an ungrounded PV panel

Do not use the instrument with circuits whose terminal-to-ground voltage exceeds 1000 V. Doing so may result in electric shock.

CM4141A961-03

# **Contents**

	ductionations	
Verif Opti	fying Package Contents ons (sold separately)ge Notes	4 5
1	Overview	11
1.1 1.2	Product Overview and Features	
2	Making Measurements	13
2.1 2.2	Inspection Before Measurement Current Measurement Manual Hold/Auto Hold	14 15
	MAX value/MIN value/AVG value/PEAK value Filter Function Rush current (AC INRUSH)	19 20 21
2.3	Other Measurement Functions	
	HIOKI CM4141A961-03	i

### Contents

2.4	Backlight/Auto Power Save (APS)	26
2.5	Power-on Option Table	
2.6	Bluetooth® Communications (only for model CM4142)	29
3	Specifications	35
3.1	General Specifications	35
3.2	Input specifications/Measurement specifications	
3.3	Accuracy Table	
	•	
4	Repairs, Inspections, and Cleaning	59
4.1	Troubleshooting	50
	Troubleshooting	
4.2	Error display	
4.3	Insert/Replace Batteries	
4.4	Cleaning	64
	9	
Inde	-	65
	-	

# Introduction

Thank you for purchasing the Hioki CM4141, CM4142 AC Clamp Meter. To obtain maximum performance from the instrument over the long term, be sure to read this manual carefully and keep it handy for future reference.

Read the separate document "Operating Precautions" carefully before using the instrument.

### **Target audience**

This manual has been written for use by individuals who use the product in question or who teach others to do so. It is assumed that the reader possesses basic electrical knowledge (equivalent to that of someone who graduated from the electrical program at a technical high school).

### **Trademark**

- Bluetooth<sup>®</sup> is a registered trademark of Bluetooth SIG, Inc.(USA). The trademark is used by HIOKI E.E. CORPORATION under license.
- · Android, Google Play, and Google Chrome are trademarks of Google, Inc.
- IOS is a registered trademark of Cisco Systems, Inc. and/or its affiliates in the United States and certain other countries.
- iPhone, iPad, iPad mini<sup>™</sup>, iPad Pro, and iPod touch are trademarks of Apple Inc.
- The App Store is a service mark of Apple Inc.
- Any other products and company names are generally either trade names, registered trademarks or trademarks of respective companies.

# **Notations**

### **Concerning Safety**

In this document, the risk seriousness and the hazard levels are classified as follows.

<b>⚠ DANGER</b>	Indicates an imminently hazardous situation that will result in death or serious injury to the operator.	IMPORTANT	Indicates information related to the operation of the instrument or maintenance tasks with which the operators must be fully familiar.
<b><u></u> MARNING</b>	Indicates a potentially hazardous situation that may result in death or serious injury to the operator.	$\Diamond$	Indicates prohibited actions.
<b>⚠</b> CAUTION	Indicates a potentially hazardous situation that may result in minor or moderate injury to the operator or damage to the instrument or malfunction.	0	Indicates an action that must be performed.

### Symbols Affixed to the Instrument

<u>^</u>	Indicates cautions and hazards. Refer to the "Usage Notes" (p.6) section of the instruction manual and the included "Operating Precautions" for more information.
4	Indicates that the instrument may be connected to or disconnected from a live conductor.

### Screen display

1 2 3 4 5 6 7 8 9 0

12|3|4|5|6|7|8|9|0

The instrument screen displays the alphanumeric characters as follows.



A different display is used in the case below.

IPEn : Wiring break detected

#### Other




Indicates a buzzer sound (either intermittent or continuous).

### Accuracy

We define measurement tolerances in terms of f.s. (full scale), rdg. (reading) and dgt. (digit) values with the following meanings:


f.s.	(maximum display value/range) The maximum displayable value. This is usually the name of the currently selected range.
rdg. (displayed value) The value currently being measured and displayed on the measuring instrument.	
dgt.	(resolution) The smallest displayable unit on a digital measuring instrument, i.e., the input value that causes the digital display to show a "1" as the least-significant digit.

# **Verifying Package Contents**

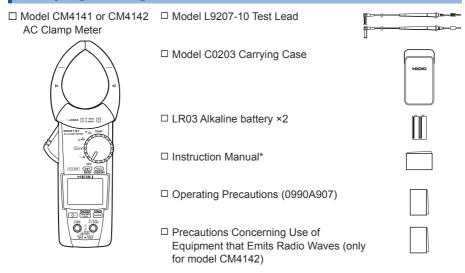

<sup>\*</sup> Instruction manuals may also be available in other languages. Please visit our website at http://www.hioki.com

# **Options (sold separately)**

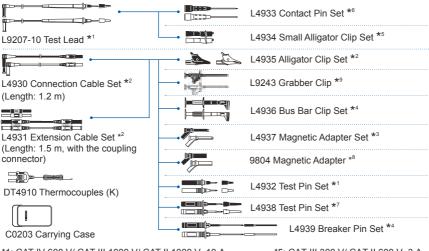

<sup>\*1:</sup> CAT IV 600 V/ CAT III 1000 V/ CAT II 1000 V, 10 A

<sup>\*2:</sup> CAT IV 600 V/ CAT III 1000 V, 10 A

<sup>\*3:</sup> CAT III 1000 V, 2 A

<sup>\*4:</sup> CAT III 600 V, 5 A

<sup>\*5:</sup> CAT III 300 V/ CAT II 600 V, 3 A

<sup>\*6: 30</sup> V AC/ 60 V DC, 3 A

<sup>\*7:</sup> CAT III 600 V/ CAT II 600 V, 10 A

<sup>\*8:</sup> CAT IV 1000 V, 2 A

# **Usage Notes**

Follow these precautions to ensure safe operation and to obtain the full benefits of the various functions. Read the separate document "Operating Precautions" carefully before using the instrument. Ensure that your use of the product falls within the specifications not only of the instrument itself, but also of any accessories, options, batteries, and other equipment being used.

# **A DANGER**

- To prevent an electric shock, do not touch any areas beyond the barrier while the instrument is in use.
   See: "Part Names" (p.12)
- The maximum measurement current varies with the frequency, and the current that can be measured continuously is limited. Operating the instrument at less than this limitation is referred to as derating. Do not measure currents in excess of the derating curve. Doing so may result in instrument damage or malfunction, a fire, or burn due to sensor heating.
- Never apply a voltage to the instrument when the resistance, continuity check, diode check, capacitance, or temperature functions are selected.
   Damage to the instrument can cause bodily injury. To avoid electrical accidents, turn off the circuit before measuring it.

# **DANGER**



 To prevent an electric shock, confirm that the white portion (insulation layer) inside the cable is not exposed. If a color inside the cable is exposed, do not use the cable.

# **MARNING**



Do not allow the instrument to get wet, and do not take measurements with wet hands. This may cause an electric shock. (This precaution does not apply to insulated conductors.)



To prevent an electric shock, do not exceed the lower of the ratings shown on the instrument and test leads.

# **A**CAUTION



Do not place any foreign object between the jaws or any insert foreign object into the gap of the sensor head. Doing so may worsen the performance of the sensor or the opening-closing operation of the sensor head.

## **CAUTION**



Avoid dropping or jarring the instrument, which could damage the jaw, adversely affecting measurement.



#### **IMPORTANT**

Clamp the instrument around only one conductor. The instrument will not be able to make a measurement if you clamp it around two or more wires together, regardless of whether they are part of a single-phase or three-phase circuit.

## **WARNING**

To prevent an electric shock, when measuring the voltage of a power line use a test lead that satisfies the following criteria:

- Conforms to safety standards IEC61010 or EN61010
- · Measurement category III or IV
- Its rated voltage is higher than the voltage to be measured
   The optional test leads provided for the instrument conform to the safety
   standard EN61010. Use a test lead in accordance with its defined measurement
   category and rated voltage.
- To prevent a short-circuit accident, be sure to use the test leads with the sleeves attached when performing measurements in the CAT III and CAT IV measurement categories.
- If the sleeves are removed during measurement, stop the measurement.

# **A**CAUTION



The cable is hardened in freezing temperatures. Do not bend or pull it to avoid tearing its shield or cutting cable.

### Model L4937, 9804 Magnetic Adapter Set (optional)

# **DANGER**



Persons wearing electronic medical devices such as a pacemaker should not use the Magnetic Adapter Set. Such persons should avoid even proximity to the Magnetic Adapter Set, as it may be dangerous. Medical device operation could be compromised, presenting a hazard to human life.

# **A CAUTION**

- Do not subject the Magnetic Adapter Set to mechanical shock, for example, due to dropping it. Shock can cause it to be chipped or cracked.
- Do not use the Magnetic Adapter Set in locations where it may be exposed to rainwater, dust, or condensation. In those conditions, the Magnetic Adapter Set may be decomposed or deteriorated. The magnet adhesion may be diminished. In such case, the instrument may not be hung in place and may fall.



 Do not bring the Magnetic Adapter Set near magnetic storage device such as floppy disks, magnetic cards, pre-paid cards, or magnetized tickets. Doing so may corrupt and may render them unusable. Furthermore, if the Magnetic Adapter Set is brought near precision electronic equipment such as PCs, TV screens, or electronic wrist watches, they may fail.

# **Overview**

### 1.1 Product Overview and Features


This instrument is a clamp meter that can perform true RMS measurement of current simply by clamping it around a circuit. In addition to current, it provides voltage measurement, frequency measurement, rush current measurement, resistance measurement, diode measurement, capacitance measurement, and temperature measurement.

Model CM4142 also provide Bluetooth® communications functionality, allowing measurement data to be monitored and logged from a mobile device.

#### Measurement function list

TEMP	Temperature
<b>≯</b> +⊣⊢	Capacitance, diode
Ω → 🚉	Continuity check, resistance
$_{ m AUTO}^{==.}\sim$ V	AUTO V, AC voltage, DC voltage, AC+DC voltage
$\sim$ A	AC current

### 1.2 Part Names

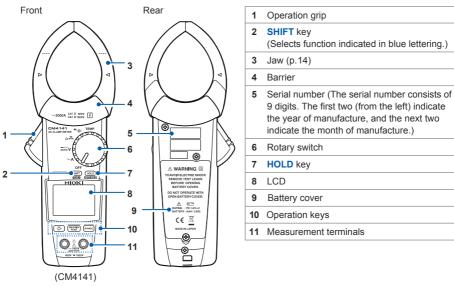



# **Making Measurements**

# 2.1 Inspection Before Measurement

Check if there is any damage to the instrument occurred during storage or shipping and verify that instrument operates normally before using it. If you find any damage, contact your authorized Hioki distributor or reseller.

Check item			
The battery cover is closed and its screw has been securely tightened.		There is no damage to the test lead insulation, and neither the white sheathing nor metal conductor inside the wire are exposed.	
There is no foreign matter on the measurement terminals. (p.12)		The instrument is neither damaged nor cracked.	
The test leads are not broken.		No indicators are missing.	
1 Ω or less		RANGE + COLOR MAX WIN MO APS GIRE  PORT TO THE WAY WIN MO APP GIRE  PORT TO THE WAY WIN MO APS GIRE  PORT TO THE WAY WIN MO APP GIRE	


## 2.2 Current Measurement

1 Turn the rotary switch.




00

Clamp the instrument around a conductor.



50.00

~5000



# Frequency detection range of AC current

3 A or more (60.00 A range) 30 A or more (600.0 A range) 200 A or more (2000 A range)

#### Range (p.18)

Default setting is auto range.

Press the **RANGE** key to switch to manual range.

Maximize measurement precision by positioning the wire on the center side of the area mark.


#### Manual Hold/Auto Hold

### Manual hold



HOLD Measured value retains.

Pressing the **HOLD** key again cancels the measured value hold function.




Measured value automatically retains.

Pressing the **HOLD** key for 1 sec. cancels the auto hold function.

#### Auto hold conditions

Display value updates are stopped when the following two conditions are satisfied:

- When the measured value exceeds the threshold value described in the table in the next page. (voltage, current). When the measured value is less than the threshold value described in the table in the next page. (resistance, continuity, diode)
- When the range over which the measured value is fluctuating stabilizes within the fluctuation range described in the table in the next page.

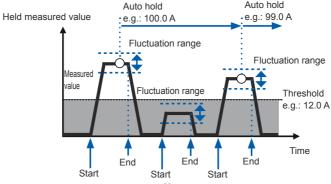


Measurement

If the measured value falls below the threshold value (voltage, current) or exceeds the threshold value (resistance, continuity, diode) after display value updates are stopped, the display value update is restarted. Display value updates will stop if the two conditions are satisfied once again.

Measurement function	Fluctuation range	Threshold value	
AC current	60.00 A range: within 400 counts 600.0 A range: within 400 counts 2000 A A range: within 40 counts	60.00 A range: 100 counts 600.0 A range: 120 counts 2000 A range: 40 counts	
AUTO V AC voltage DC voltage AC+DC voltage	6.000 V/60.00 V/600.0 V range: within 120 within 1000 V range: within 20 counts 1500 V range: within 30 counts	6.000 V/60.00 V/600.0 Vrange: 120 counts 1000 V range: 20 counts 1500 V range: 30 counts	
Resistance Continuity	600.0 $\Omega$ /6.000 k $\Omega$ /60.00 k $\Omega$ /600.0 k $\Omega$ range: within 100 counts	600.0 $\Omega$ /6.000 k $\Omega$ /60.00 k $\Omega$ /600.0 k $\Omega$ range: 4900 counts	
Diode	1.800 V range: within 40 counts	1.800 V range: 1460 counts	

The auto hold function only operates for the above measurement functions.

### Switching the range

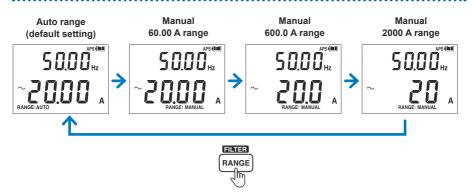


19


### MAX value/MIN value/AVG value/PEAK value

Clamp the instrument around a conductor. FILTER See: "Switching the range" (p.18) RANGE In auto-range mode, the instrument will be automatically set to the 2000 A range. **AC INRUSH** MAX/MIN MAX → MIN → AVG → PEAK MAX **→ PEAK** MIN PEAK o MAX/MIN PEAK Press for 1 sec. Cancel HOLD \$\( \square\) Measured value retains. AUTO HOLD PEAK MAX MAX The instrument Waveform performs true RMS Measured value measurement (RMS value) 9 9 "AVG" indicates the average of all PEAK MIN measured values Display refresh interval HIOKI CM4141A961-03

#### **Filter Function**

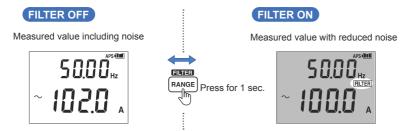

# Frequency characteristics when using the filter function (100 A input)




Turn off the filter function when performing measurement of power supply frequencies in excess of 100 Hz, for example on an aircraft or ship.

## **Rush current (AC INRUSH)**

- 1 Turn off the motor.
- 2 Turn the rotary switch.



3 Clamp the instrument around a conductor



4 Set the range.

RANGE In auto-range mode, the instrument will be automatically set to the 2000 A range.


HIOKI CM4141A961-03

Press for 1 sec.




Turn on the motor.

The instrument can measure AC rush current. Rush current containing a DC component cannot be measured accurately.



(Rush current occurrence)





## Trigger level

±2 A peak (60.00 A range) ±10 A peak (600.0 A range) ±100 A peak (2000 A range)


Interval during which rush current occurs (Dozens to hundreds of milliseconds in duration)


21

## 2.3 Other Measurement Functions


### **Voltage**

e.g.: commercial power supply (AC voltage measurement)

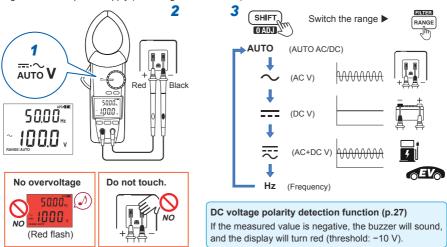

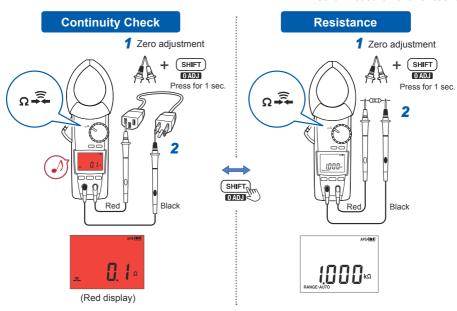


#### Other Measurement Functions

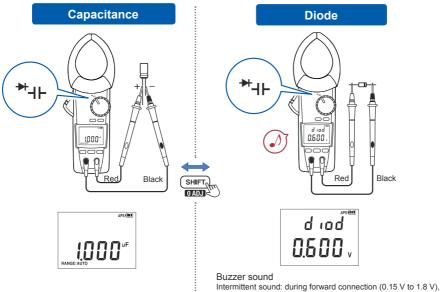

backlight off


Continuous sound: during forward connection (less than 0.15 V), red backlight on

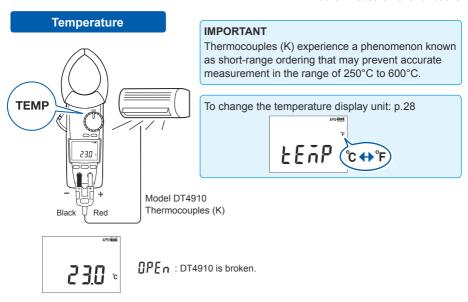

# 2.4 Backlight/Auto Power Save (APS)



Backlight ON Automatically switched off when the instrument is not in use for 40 sec. (Automatic backlight deactivation ON) Cancelation method: p.27



HIOKI CM4141A961-03

# 2.5 Power-on Option Table



Move the rotary switch from the "OFF" position to any of the test mode positions while pressing an operation key.

Setting	Operating instruction	Factory setting	Setting retained?
Canceling the auto power save (APS) function (OFF)	HOLD +	ON	No (Set each time)
DC voltage polarity detection function (ON/OFF)	SHIFT +	OFF	Yes
Displaying all indicators (Version of software/Model number/ Serial number)	RANGE +	-	-
Buzzer sound (ON/OFF)	MAX/MIN +	ON	Yes
Automatic backlight deactivation (ON/OFF)	÷ (	ON	Yes

### Power-on Option Table


Setting	Operating instruction	Factory setting	Setting retained?
Switching the temperature unit	SHIFT + (HOLD) + (MAX/MIN) + (RANGE) Press for 1 sec.	°C	V
Switching the temperature unit	To change the temperature unit:  RANGE  To save the setting:  MAX/MIN PEAK  Press for 1 sec.	C	Yes

# 2.6 Bluetooth® Communications (only for model CM4142)

The CM4142 supports Bluetooth (Bluetooth low energy). When the Bluetooth function is enabled, you can review measurement data and create measurement reports on mobile devices (iPhone, iPad, iPad mini $^{\text{TM}}$ , iPad Pro, iPod touch, and Android $^{\text{TM}}$  devices). For more information about this functionality, see the **Help** function in the application software GENNECT Cross.

- 1 Install the GENNECT Cross on your mobile device. (p.30)
- 2 Enable the Bluetooth function on the CM4142. (p.31)
- 3 Launch the GENNECT Cross and pair it with the CM4142. (p.32)
- 4 Select the General Measurement, Logging (Recording), or Waveform/FFT function. (p.33)







### Bluetooth® Communications (only for model CM4142)

### Installing the application software GENNECT Cross

Search for "GENNECT Cross" on the App Store from your iPhone, iPad or other Apple device, or on Google Play<sup>TM</sup> from your Android device. Then download and install the GENNECT Cross. You will need an Apple ID to download the app on the App Store, or a Google account to download the app on Google Play. For more information about how to register an account, contact the store at which you purchased your device.








- Because the CM4142 emit radio waves, use in a country or region where they have not been approved may
  be subject to fines or other penalties as a violation of applicable laws or regulations. For more information,
  see the attached "Precautions Concerning Use of Equipment that Emits Radio Waves" or go to our website.
- The CM4142 availability is limited to certain countries. For more information, contact your authorized Hioki distributor or reseller.
- The distance over which data can be sent and received using Bluetooth varies greatly depending on
  whether there are any obstructions between the paired instruments (for example, walls, metal barriers, etc.)
  and on the distance between the instrument and the floor (or ground). To ensure stable measurement, verify
  adequate signal strength.
- Although this application software is provided free of charge, downloading or using the application software may incur Internet connection charges. Such charges are the sole responsibility of the user.
- This application software is not guaranteed to operate on all mobile devices.

#### **Turning on the Bluetooth function**







Press for 1 sec.

#### Bluetooth function ON



- lights up: Bluetooth function ON
- flashes: Sending/receiving data

#### Bluetooth® Communications (only for model CM4142)

#### Pairing the app with the CM4142



- When the app is launched for the first time (before being paired with any instrument), the Instrument Settings screen will be displayed.
- While the mobile device is displaying the **Instrument Settings** screen, simply move it close to a CM4142 to automatically pair it with the instrument (the app can be paired with up to 8 instruments).
- Allow about 5 to 30 seconds for the CM4142 to pair with the app after being turned on. If the instrument fails
  to pair within 1 minute, relaunch GENNECT Cross and cycle the instrument's power.

#### Making measurements with the Bluetooth function

Select the **General Measurement**, **Logging (Recording)**, or **Waveform/FFT** function on the **Home** screen. For more information about each function, see the **Help** function in the GENNECT Cross.



**General Measurement** 

Saves measured values from multiple channels



Logging (Recording)

Simple logging (up to 24 hours)



Waveform/FFT

Simple oscilloscope (voltage/current)

Bluetooth® Communications (only for model CM4142)

#### 3

# **Specifications**

#### 3.1 General Specifications

Operating environment	Indoors, pollution degree 2, altitude up to 2000 m (6562 ft.)		
Operating temperature and humidity	-25°C to 65°C (-13°F to 149°F), 90% RH or less (no condensation)		
Storage temperature and humidity	-30°C to 70°C (-22°F to 158°F), 90% RH or less (no condensation, when batteries are removed)		
Dustproof and waterproof	IP20 (Measuring voltage or current in a hazardous live conductor while completely dry) IP50 (Measuring resistance or current in an insulated conductor while completely dry, or during storage) However, the instrument's handle provides IP54-equivalent dust and water protection when the instrument is not making a measurement.		
Standards	Safety EN 61010 EMC EN 61326		
Power supply	LR03 alkaline battery ×2 Rated supply voltage: 1.5 V DC ×2		
Continuous operating time	Approx. 48 hours (Bluetooth communication OFF) Approx. 24 hours (Bluetooth communication ON) Other conditions: 100 A AC measurement, LCD backlight OFF, at 23°C (73.4°F), for reference		

#### **General Specifications**

Interface (only for CM4142)	Bluetooth 4.0 LE Bluetooth (p.29)
Dimensions	Approx. 65W × 247H × 35D mm (2.56"W × 9.72"H × 1.38"D) (excluding protruding parts, operation grip, and jaw)
Jaw dimensions	Approx. 82W $\times$ 11D mm (3.23"W $\times$ 0.43"D) (The D figure indicates the depth for the first 44 mm of each jaw from its tip.)
Jaw cross-sectional minimum dimension	Approx. 11 mm (0.43") (Indicates the depth for the first 44 mm of each jaw from its tip.)
Maximum measurable conductor diameter	φ55 mm (2.17")
Mass	Approx. 300 g (10.6 oz.) (including batteries)
Product warranty period	3 years Number of jaw open/close cycles: 30,000
Accessories	See: "Verifying Package Contents" (p.4)
Options	See: "Options (sold separately)" (p.5)

#### 3.2 Input specifications/Measurement specifications

#### (1) Basic Specifications

Measurement range	See "3.3 Accuracy Table" (p.44)			
Maximum input current	As per frequency derating (p.38)			
Maximum input voltage	to terminal	600 V AC (Measurement category IV) 1000 V AC (Measurement category III) 1000 V AC (up to 1 kHz) 1700 V DC		
	to earth  600 V AC (Measurement category I'  1000 V AC (Measurement category Anticipated transient overvoltage: 8			
Measurement method	True RMS measurement			
Measurement terminals	COM terminal and V terminal			
Coupling type	AC current/current frequency/ AC INRUSH/AC voltage*1/ voltage frequency	AC coupling		
	Measurement items other than the above	DC coupling		

#### Input specifications/Measurement specifications

Display update rate *2	AC current/AUTO V/AC voltage/ DC voltage/AC+DC voltage	5 times/sec.
	Current frequency/ voltage frequency/capacitance	0.5 times to 5 times/sec. (varies depending on the measurement value.)
	Temperature (Thermocouples [K])	1 time/sec.

<sup>\*1:</sup> Does not apply to AC detection in AUTO V mode or to the AC component when DC+AC voltage are mixed.

#### (2) Current measurement specifications

Frequency derating	Lower of 3000 A AC or 6×10 <sup>6</sup> A·Hz (continuous, design value)			
Zero-display range	AC current	current 5 counts or less		
Crest factor	AC current/ AC INRUSH	60.00 A range 600.0 A range	3 (5000 counts or less) 2.5 (more than 5000 counts, 6000 counts or less)	
		2000 A range	1.5 (2000 counts or less)	
Frequency detection input level	AC current/ current frequency	60.00 A range 600.0 A range	300 counts or more	
		2000 A range	200 counts or more	

<sup>\*2:</sup> Does not include range change time.

AC INRUSH Trigger level  AC INRUSH		60.00 A range	+2.0 A <sub>PEAK</sub> or more, or -2.0 A <sub>PEAK</sub> or less
		600.0 A range	+10 A $_{PEAK}$ or more, or -10 A $_{PEAK}$ or less
		2000 A range	+100 A $_{\text{PEAK}}$ or more, or -100 A $_{\text{PEAK}}$ or less
Peak detection time width	AC current/ AC INRUSH	1 ms or more (when filter is off)	

#### (3) Voltage measurement specifications

Overload protection	1870 V DC Lower of 1100 V AC or 2×10 <sup>7</sup> V·Hz (Applied continuously for up to 1 min.)			
Input impedance	See "3.3 Accuracy Table"	" (p.44)		
Zero-display range	AUTO V/AC voltage/ AC+DC voltage	5 counts or less		
Crest factor	AUTO V/AC voltage/ AC+DC voltage	6.000 V range 60.00 V range 600.0 V range	3 (4000 counts or less) 2 (more than 4000 counts, 6000 counts or less)	
		1000 V range	2 (850 counts or less) 1.7 (more than 850 counts, 1000 counts or less)	

#### Input specifications/Measurement specifications

Frequency detection input level	AUTO V/AC voltage	10% or more of each range f.s.
CMRR *1	AC voltage/AC+DC voltage	-60 dB or more
	DC voltage	−100 dB or more
NMRR *2	DC voltage	−60 dB or more
Peak detection time width	AC voltage	1 ms or more (when filter is off)

<sup>\*1:</sup> Defined for 1 k $\Omega$  unbalance, 0 Hz/50 Hz/60 Hz input

#### (4) Other Measurement Specifications

Overload protection	1700 V DC Lower of 1000 V AC or 2×10 <sup>7</sup> V·Hz (Applied continuously for up to 1 min.)
Overload current	At steady state: 30 mA or less At transient state: 1.5 A or less
Measurement current/charging current	See "3.3 Accuracy Table" (p.44)

<sup>\*2:</sup> Defined for 50 Hz/60 Hz input

Open terminal voltage	2.0 V DC or less	
Continuity on threshold	Continuity check	25 $\Omega\pm10~\Omega$ (continuous buzzer sound, red warning backlight lights up)
Continuity off threshold	Continuity check	245 Ω±10 Ω
Maximum capacity load	Resistance	10 mF
Maximum inductive load	Resistance	10 H
Instrument reference contact temperature correction stabilization time	Temperature (Thermocouples [K])	Up to 120 minutes (Reference: For an instrument at 23°C [73°F] placed in a 65°C [149°F] environment: 60 minutes)

#### (5) Accuracy specifications

Conditions of guaranteed accuracy	Guaranteed accuracy period	1 year (accuracy shown in accuracy table) 3 years (accuracy shown in accuracy table ×1.5) (reference values)		
	Guaranteed accuracy period after adjustment made by Hioki	1 year		
	Guaranteed accuracy for temperature and humidity	23°C±5°C (73°F±9°F), 90% RH or less (no condensation)		
	Continuity check/resistance: after zero adjustment has been performed Use model DT4910 for temperature (Thermocouples [K])			
Conditions of accuracy input	Sine wave input			
Measurement accuracy	See "3.3 Accuracy Table" (p.44)			
Temperature coefficient	Add "measurement accura	acy × 0.1/°C" (excluding 23°C±5°C [73°F±9°F]).		

Effects of conductor position *1	Cable diameter	Measurement area	Accuracy	Measurement area figure
	CV8 mm <sup>2</sup>	Area A	Within ±3.0% rdg.	
	(Finished outer diameter: 8.6 mm)	Area B	Within ±7.0% rdg.	B
	CV38 mm² (Finished outer diameter: 13 mm)	Area A	Within ±2.0% rdg.	
		Area B	Within ±5.0% rdg.	
Effect of radiated radio-frequency electromagnetic	Add ±2% rdg. at 10 V/m.			

<sup>\*1:</sup> At 100 A, 55 Hz measurements around the jaw's center-point reference

field

#### 3.3 Accuracy Table

#### (1) AC current

#### Measurement value/MAX/MIN/AVE (rms)

Range	Accuracy	Accuracy	Measurement accuracy		
(Auto-range threshold)	guarantee range (Resolution)			Filter ON*1	
60.00 A	1.00 A to 60.00 A	45 Hz ≤ f ≤ 66 Hz	±1.5% rdg.±0.08 A	±2.0% rdg.±0.08 A	
(more than 6000 counts)	(0.01 A)	30 Hz ≤ f < 45 Hz, 66 Hz < f ≤ 1 kHz	±2.0% rdg.±0.10 A	±2.5% rdg.±0.10 A	
600.0 A	1.0 A to 600.0 A	45 Hz ≤ f ≤ 66 Hz	±1.5% rdg.±0.3 A	±2.0% rdg.±0.3 A	
(more than 6000 counts/ less than 540 counts)	(0.1 A)	30 Hz ≤ f < 45 Hz, 66 Hz <f 1="" khz<="" td="" ≤=""><td>±2.0% rdg.±0.5 A</td><td>±2.5% rdg.±0.5 A</td></f>	±2.0% rdg.±0.5 A	±2.5% rdg.±0.5 A	
2000 A	10 A to 2000 A	45 Hz ≤ f ≤ 66 Hz	±1.5% rdg.±3 A	±2.0% rdg.±3 A	
(less than 540 counts)	(1 A)	30 Hz ≤ f < 45 Hz, 66 Hz <f 1="" khz*<sup="" ≤="">2</f>	±2.0% rdg.±5 A	±2.5% rdg.±5 A	

<sup>\*1:</sup> Accuracy not defined beyond 66 Hz.

<sup>\*2:</sup> Design values apply beyond 6×10<sup>5</sup> A⋅Hz.

#### PEAK MAX/PEAK MIN (Zero to Peak)

Range	Accuracy guarantee range (Resolution)	Accuracy guarantee frequency range	Measurement accuracy
60.00 A	±1.0 A to ±150.0 A	45 Hz ≤ f ≤ 66 Hz	±1.5% rdg.±0.8 A
	(0.1 A)	30 Hz ≤ f < 45 Hz, 66 Hz < f ≤ 1 kHz	±2.0% rdg.±1.0 A
600.0 A	±10 A to ±1500 A	45 Hz ≤ f ≤ 66 Hz	±1.5% rdg.±3 A
	(1 A)	30 Hz ≤ f < 45 Hz, 66 Hz < f ≤ 1 kHz	±2.0% rdg.±5 A
2000 A	±10 A to ±2840 A	45 Hz ≤ f ≤ 66 Hz	±1.5% rdg.±30 A
	(1 A)	30 Hz ≤ f < 45 Hz, 66 Hz < f ≤ 1 kHz	±2.0% rdg.±50 A

#### (2) Current frequency

Range (Auto-range threshold)	Accuracy guarantee range (Resolution)	Measurement accuracy
99.99 Hz (more than 9999 counts)	30.00 Hz to 99.99 Hz (0.01 Hz)	±0.1% rdg.±0.01 Hz
999.9 Hz (less than 900 counts)	30.0 Hz to 999.9 Hz (0.1 Hz)	±0.1% rdg.±0.1 Hz*1

<sup>\*1:</sup> Add ±0.2 Hz if less than 100.0 Hz.

#### (3) AC INRUSH (Rush current)

#### AC INRUSH measurement value (rms)

Range	Accuracy guarantee range (Resolution)	Accuracy guarantee frequency range	Measurement accuracy
60.00 A	3.00 A to 60.00 A (0.01 A)	40 Hz ≤ f ≤ 500 Hz	±5.0% rdg.±0.13 A
600.0 A	10.0 A to 600.0 A (0.1 A)	40 Hz ≤ f ≤ 500 Hz	±5.0% rdg.±1.3 A
2000 A	100 A to 2000 A (1 A)	40 Hz ≤ f ≤ 500 Hz*1	±5.0% rdg.±13 A

<sup>\*1:</sup> Design values apply beyond 6×10<sup>5</sup> A·Hz.

#### AC INRUSH PEAK value (Zero to Peak)

Range	Accuracy guarantee range (Resolution)	Accuracy guarantee frequency range	Measurement accuracy
60.00 A	3.0 A to 150.0 A (0.1 A)	40 Hz ≤ f ≤ 500 Hz	±5.0% rdg.±1.0 A
600.0 A	10 A to 1500 A (1 A)	40 Hz ≤ f ≤ 500 Hz	±5.0% rdg.±10 A
2000 A	100 A to 2840 A (10 A)	40 Hz ≤ f ≤ 500 Hz	±5.0% rdg.±100 A

#### (4) AUTO V (AC/DC voltage automatic detection)

During AC detection: Conforms to accuracy specifications described in "(7) AC+DC voltage" (p.52). During DC detection: Conforms to accuracy specifications described in "(6) DC voltage" (p.50).

#### (5) AC voltage

#### Measurement value/MAX/MIN/AVE

Range	Accuracy	Accuracy quarantee Measurement accuracy		Input	
(Auto-range threshold)	guarantee range (Resolution)	frequency range *1 *2	Filter OFF	Filter ON	impedance *3
6.000 V (more than 6000	0.000 V to 0.299 V (0.001 V)	15 Hz ≤ f < 45 Hz	±1.5% rdg. ±0.015 V	±2.0% rdg. ±0.015 V	3.2 MΩ±5%
counts)		45 Hz ≤ f ≤ 66 Hz	±0.9% rdg. ±0.013 V	±1.4% rdg. ±0.013 V	
		66 Hz < f ≤ 1 kHz	±1.5% rdg. ±0.015 V	_	
	0.300 V to 6.000 V (0.001 V)	15 Hz ≤ f < 45 Hz	±1.5% rdg. ±0.005 V	±2.0% rdg. ±0.005 V	3.2 MΩ±5%
		45 Hz ≤ f ≤ 66 Hz	±0.9% rdg. ±0.003 V	±1.4% rdg. ±0.003 V	
		66 Hz < f ≤ 1 kHz	±1.5% rdg. ±0.005 V	_	

#### Accuracy Table

Range	Accuracy	Accuracy guarantee	Measuremen	nt accuracy	Input
(Auto-range threshold)	guarantee range (Resolution)	frequency range *1 *2	Filter OFF	Filter ON	impedance *3
60.00 V (more than	3.00 V to 60.00 V (0.01 V)	15 Hz ≤ f < 45 Hz	±1.5% rdg. ±0.05 V	±2.0% rdg. ±0.05 V	3.1 MΩ±5%
6000 counts/ less than 540		45 Hz ≤ f ≤ 66 Hz	±0.9% rdg. ±0.03 V	±1.4% rdg. ±0.03 V	
counts)		66 Hz < f ≤ 1 kHz	±1.5% rdg. ±0.05 V	_	
600.0 V (more than	30.0 V to 600.0 V (0.1 V)	15 Hz ≤ f < 45 Hz	±1.5% rdg. ±0.5 V	±2.0% rdg. ±0.5 V	3.0 MΩ±5%
6000 counts/ less than 540		45 Hz ≤ f ≤ 66 Hz	±0.9% rdg. ±0.3 V	±1.4% rdg. ±0.3 V	
counts)		66 Hz < f ≤ 1 kHz	±1.5% rdg. ±0.5 V	_	
1000 V (less than 540	50 V to 1000 V (1 V)	15 Hz ≤ f < 45 Hz	±1.5% rdg. ±5 V	±2.0% rdg. ±5 V	3.0 MΩ±5%
counts)		45 Hz ≤ f ≤ 66 Hz	±0.9% rdg. ±3 V	±1.4% rdg. ±3 V	
		66 Hz < f ≤ 1 kHz	±1.5% rdg. ±5 V	_	

<sup>\*1:</sup> Frequency range of 15 Hz  $\leq$  f < 20 Hz is designed value.

<sup>\*2:</sup> Within the frequency range of f < 45 Hz, the accuracy guarantee assumes a superposed DC voltage of less than 500 V.

<sup>\*3:</sup>At 50 Hz AC.

#### PEAK MAX/PEAK MIN

Range	Accuracy guarantee range (Resolution)	Accuracy guarantee frequency range *1 *2	Measurement accuracy
6.000 V	0 V to ±12.00 V (0.01 V)	15 Hz ≤ f < 45 Hz	±1.8% rdg.±0.07 V
		45 Hz ≤ f ≤ 66 Hz	±1.5% rdg.±0.07 V
		66 Hz < f ≤ 1 kHz	±1.8% rdg.±0.07 V
60.00 V	±3.0 V to ±120.0 V (0.1 V)	15 Hz ≤ f < 45 Hz	±1.8% rdg.±0.7 V
		45 Hz ≤ f ≤ 66 Hz	±1.5% rdg.±0.7 V
		66 Hz < f ≤ 1 kHz	±1.8% rdg.±0.7 V
600.0 V	±30 V to ±1000 V *3 (1 V)	15 Hz ≤ f < 45 Hz	±1.8% rdg.±7 V
		45 Hz ≤ f ≤ 66 Hz	±1.5% rdg.±7 V
		66 Hz < f ≤ 1 kHz	±1.8% rdg.±7 V
1000 V	±50 V to ±1000 V *4 (1 V)	15 Hz ≤ f < 45 Hz	±1.8% rdg.±7 V
		45 Hz ≤ f ≤ 66 Hz	±1.5% rdg.±7 V
		66 Hz < f ≤ 1 kHz	±1.8% rdg.±7 V

<sup>\*1:</sup> Frequency range of 15 Hz  $\leq$  f < 20 Hz is designed value.

<sup>\*2:</sup> Within the frequency range of f < 45 Hz, the accuracy guarantee assumes a superposed DC voltage of less than 500 V.

<sup>\*3:</sup> Values of up to ±1200 V are displayed, but accuracy is not defined for display values in excess of 1000 V (which are provided as reference values).

<sup>\*4:</sup> Values of up to ±1700 V are displayed, but accuracy is not defined for display values in excess of 1000 V (which are provided as reference values).

#### Accuracy Table

#### (6) DC voltage

#### Measurement value/MAX/MIN/AVE

Range (Auto-range threshold)	Accuracy guarantee range (Resolution)	Measurement accuracy	Input impedance*1
600.0 mV	0.0 mV to ±600.0 mV	±0.5% rdg.	6.7 MΩ±5%
(more than 6000 counts)	(0.1 mV)	±0.5 mV	
6.000 V (more than 6000 counts/	0.000 V to ±6.000 V	±0.5% rdg.	6.7 MΩ±5%
less than 540 counts)	(0.001 V)	±0.003 V	
60.00 V (more than 6000 counts/	0.00 V to ±60.00 V	±0.5% rdg.	6.1 MΩ±5%
less than 540 counts)	(0.01 V)	±0.03 V	
600.0 V (more than 6000 counts/	0.0 V to ±600.0 V	±0.5% rdg.	6.0 MΩ±5%
less than 540 counts)	(0.1 V)	±0.3 V	
1500 V (less than 540 counts)	0 V to ±1000 V * <sup>2</sup> (1 V)	±0.5% rdg. ±3 V	6.0 MΩ±5%
	±1001 V to ±1700 V * <sup>2</sup> (1 V)	±2.0% rdg. ±5 V	

<sup>\*1:</sup>At DC input

<sup>\*2:</sup> In the 1500 V range, the instrument can withstand input of up to 1000 V continuously or input in excess of 1000 V for no greater than 1 minute.

#### **PEAK MAX/PEAK MIN**

Range	Accuracy guarantee range (Resolution)	Measurement accuracy
600.0 mV	0 mV to ±1200 mV (1 mV)	±1.0% rdg.±7 mV
6.000 V	0.00 V to ±12.00 V (0.01 V)	±1.0% rdg.±0.07 V
60.00 V	0.0 V to ±120.0 V (0.1 V)	±1.0% rdg.±0.7 V
600.0 V	0 V to ±1000 V (1 V)	±1.0% rdg.±7 V
	±1001 V to ±1200 V (1 V)	±5.0% rdg.±7 V
1500 V	0 V to ±1000 V (1 V)	±1.0% rdg.±7 V
	±1001 V to ±1700 V (1 V)	±5.0% rdg.±7 V

#### (7) AC+DC voltage

#### Measurement value/MAX/MIN/AVE

Range	Accuracy	Accuracy guarantee	Measureme	nt accuracy	Input
(Auto-range threshold)	guarantee range (Resolution)	frequency range *1	Filter OFF	Filter ON	impedance *2
6.000 V (more than 6000	0.000 V to 0.299 V (0.001 V)	10 Hz ≤ f < 45 Hz	±1.5% rdg. ±0.023 V	±2.0% rdg. ±0.023 V	DC: 6.7 MΩ±5% AC: 3.2 MΩ±5%
counts)		DC, 45 Hz ≤ f ≤ 66 Hz	±1.0% rdg. ±0.023 V	±1.5% rdg. ±0.023 V	
		66 Hz < f ≤ 1 kHz	±1.5% rdg. ±0.023 V	_	
	0.300 V to 6.000 V (0.001 V)	10 Hz ≤ f < 45 Hz	±1.5% rdg. ±0.013 V	±2.0% rdg. ±0.013 V	DC: 6.7 MΩ±5% AC: 3.2 MΩ±5%
		DC, 45 Hz ≤ f ≤ 66 Hz	±1.0% rdg. ±0.013 V	±1.5% rdg. ±0.013 V	
		66 Hz < f ≤ 1 kHz	±1.5% rdg. ±0.013 V	_	
60.00 V (more than	3.00 V to 60.00 V (0.01 V)	10 Hz ≤ f < 45 Hz	±1.5% rdg. ±0.13 V	±2.0% rdg. ±0.13 V	DC: 6.1 MΩ±5% AC: 3.1 MΩ±5%
6000 counts/ less than 540		DC, 45 Hz ≤ f ≤ 66 Hz	±1.0% rdg. ±0.13 V	±1.5 %rdg. ±0.13 V	
counts)		66 Hz < f ≤ 1 kHz	±1.5% rdg. ±0.13 V	_	

Range	Accuracy	Accuracy guarantee	Measureme	nt accuracy	Input
(Auto-range threshold)	guarantee range (Resolution)	frequency range *1	Filter OFF	Filter ON	impedance *2
600.0 V (more than	30.0 V to 600.0 V (0.1 V)	10 Hz ≤ f < 45 Hz	±1.5% rdg. ±0.7 V	±2.0% rdg. ±0.7 V	DC: 6.0 MΩ±5% AC: 3.0 MΩ±5%
6000 counts/ less than 540		DC, 45 Hz ≤ f ≤ 66 Hz	±1.0% rdg. ±0.7 V	±1.5% rdg. ±0.7 V	
counts)		66 Hz < f ≤ 1 kHz	±1.5% rdg. ±0.7 V	_	
1000 V (less than 540	50 V to 1000 V (1 V)	10 Hz ≤ f < 45 Hz	±1.5 %rdg. ±7 V	±2.0 %rdg. ±7 V	DC: 6.0 MΩ±5% AC: 3.0 MΩ±5%
counts)		DC, 45 Hz ≤ f ≤ 66 Hz	±1.0 %rdg. ±7 V	±1.5 %rdg. ±7 V	
		66 Hz < f ≤ 1 kHz	±1.5 %rdg. ±7 V	-	

<sup>\*1:</sup> Frequency range of 10 Hz  $\leq$  f < 20 Hz is designed value.

<sup>\*2:</sup> At DC input, 50 Hz AC input.

#### Accuracy Table

#### PEAK MAX/PEAK MIN

Range	Accuracy guarantee range (Resolution)	Accuracy guarantee frequency range *1	Measurement accuracy
6.000 V	0.00 V to ±12.00 V	10 Hz ≤ f < 45 Hz	±1.5% rdg.±0.07 V
	(0.01 V)	DC, 45 Hz ≤ f ≤ 66 Hz	±1.0% rdg.±0.07 V
		66 Hz < f ≤ 1 kHz	±1.5% rdg.±0.07 V
60.00 V	±3.0 V to ±120.0 V	10 Hz ≤ f < 45 Hz	±1.5% rdg.±0.7 V
	(0.1 V)	DC, 45 Hz ≤ f ≤ 66 Hz	±1.0% rdg.±0.7 V
		66 Hz < f ≤ 1 kHz	±1.5% rdg.±0.7 V
600.0 V	±30 V to ±1000 V *2	10 Hz ≤ f < 45 Hz	±1.5% rdg.±7 V
	(1 V)	DC, 45 Hz ≤ f ≤ 66 Hz	±1.0% rdg.±7 V
		66 Hz < f ≤ 1 kHz	±1.5% rdg.±7 V
1000 V	±50 V to ±1000 V *3	10 Hz ≤ f < 45 Hz	±1.5% rdg.±7 V
	(1 V)	DC, 45 Hz ≤ f ≤ 66 Hz	±1.0% rdg.±7 V
		66 Hz < f ≤ 1 kHz	±1.5% rdg.±7 V

<sup>\*1:</sup> Frequency range of 10 Hz ≤ f < 20 Hz is designed value.

<sup>\*2:</sup> Values of up to ±1200 V are displayed, but accuracy is not defined for display values in excess of 1000 V (which are provided as reference values).

<sup>\*3:</sup> Values of up to ±1700 V are displayed, but accuracy is not defined for display values in excess of 1000 V (which are provided as reference values).

#### (8) Voltage frequency

Range (Auto-range threshold)	Accuracy guarantee range (Resolution)	Measurement accuracy
9.999 Hz (more than 9999 counts	1.000 Hz to 9.999 Hz (0.001 Hz)	±0.1% rdg.±0.003 Hz
99.99 Hz (more than 9999 counts/less than 900 counts)	1.00 Hz to 99.99 Hz (0.01 Hz)	±0.1% rdg.±0.01 Hz
999.9 Hz (less than 900 counts)	1.0 Hz to 999.9 Hz (0.1 Hz)	±0.1% rdg.±0.1 Hz*1

<sup>\*1:</sup> Add ±0.2 Hz if less than 100.0 Hz.

#### (9) Continuity check

Range	Accuracy guarantee range (Resolution)	Measurement current	Measurement accuracy
600.0 Ω	0.0 Ω to 600.0 Ω (0.1 Ω)	200 μA±20%	±0.7% rdg.±0.5 Ω

#### Accuracy Table

#### (10) Resistance

Range (Auto-range threshold)	Accuracy guarantee range (Resolution)	Measurement current	Measurement accuracy
600.0 Ω	0.0 Ω to 600.0 Ω	200 μA±20%	±0.7% rdg.
(more than 6000 counts)	(0.1 Ω)		±0.5 Ω
6.000 kΩ	0.000 k $\Omega$ to 6.000 k $\Omega$	100 μA±20%	±0.7% rdg.
(more than 6000 counts/less than 540 counts)	(0.001 kΩ)		±0.005 kΩ
60.00 kΩ	$0.00~\text{k}\Omega$ to $60.00~\text{k}\Omega$	10 μA±20%	±0.7% rdg.
(more than 6000 counts/less than 540 counts)	(0.01 kΩ)		±0.05 kΩ
600.0 kΩ	0.0 kΩ to 600.0 kΩ	1 μA±20%	±0.7% rdg.
(less than 540 counts)	(0.1 kΩ)		±0.5 kΩ

#### (11) Diode

Range	Accuracy guarantee range (Resolution)	Short-circuit current	Measurement accuracy
1.800 V	0.000 V to 1.800 V *1 (0.001 V)	200 μA±20%	±0.7% rdg.±0.005 V

<sup>\*1:</sup> Beeping buzzer tone at forward connection (0.15 V to 1.8 V). Continuous buzzer tone and red backlight lights up if less than 0.15 V.

#### (12) Capacitance

Range (Auto-range threshold)	Accuracy guarantee range (Resolution)	Discharge current	Measurement accuracy
1.000 µF	0.000 μF to 1.100 μF	10 nA±20%	±1.9% rdg.
(more than 1100 counts)	(0.001 μF)	100 nA±20%	±0.005 µF
		1 μA±20%	
10.00 μF	0.00 μF to 11.00 μF	100 nA±20%	±1.9% rdg.
(more than 1100 counts/less than	(0.01 µF)	1 μA±20%	±0.05 µF
100 counts)		10 μA±20%	
100.0 μF	0.0 μF to 110.0 μF	1 μA±20%	±1.9% rdg.
(more than 1100 counts/less than	(0.1 μF)	10 μA±20%	±0.5 µF
100 counts)		100 μA±20%	
1000 μF	0 μF to 1100 μF	10 μA±20%	±1.9% rdg.
(less than 100 counts)	(1 µF)	100 μA±20%	±5 µF
		200 µA±20%	

#### (13) Temperature (Thermocouples (K))

Range Accuracy guarantee range (Resolution) Measure		Measurement accuracy *1
°C	-40.0°C to 400.0°C (0.1°C)	±0.5% rdg.±3.0°C
°F *2	-40.0°F to 752.0°F (0.1°F)	±0.5% rdg.±5.4°F

<sup>\*1:</sup> Conditions (In an environment where the temperature of the instrument is  $\pm 1^{\circ}$ C and stable)

 $<sup>^{\</sup>star}2$ : Instrument can be made to display readings in Fahrenheit ( $^{\circ}F$ ) by means of special operation.

Accuracy Table



#### Repairs, Inspections, and Cleaning

#### 4.1 Troubleshooting

Symptom	Verification and/or Solution
The instrument is indicating an abnormal measured value.	<ul> <li>Is the measured current value too small for the instrument's measurement range?</li> <li>Wrap the wire around the jaw one or more times. Each additional wrap of the wire will increase the measured value, so that wrapping it once yields a measured value that is twice the actual value and wrapping it twice yields a measured value that is three times the actual value.</li> </ul>
	Is the tip of the jaw open?
	Is the jaw damaged?     If the jaw is damaged or cracked, it will not be able to measure current accurately. Send the instrument for repair.
	Displayed values can frequently fluctuate due to induction potential even when no voltage is applied. This, however, is not a malfunction.

#### Troubleshooting

Symptom	Verification and/or Solution
When readings from the instrument are compared with those of another clamp-on current meter, the measured values differ.	The instrument cannot accurately measure waveforms that contain a component that falls outside the frequency characteristics range.
	Since the instrument performs true RMS measurement, it can accurately measure distorted waveforms. When measuring a distorted waveform, the measured value will differ from a clamp-on current meter that uses the averaging method.
<ul> <li>The current value is larger than expected.</li> <li>A current value is displayed even though there is no input.</li> </ul>	The instrument cannot perform measurement accurately in the presence of a strong magnetic field from a source such as a nearby transformer or high-current circuit or in the presence of a strong electric field from a source such as a wireless device.  If there are any wires carrying a large current near the tip of the jaws (on the outside of the jaws), the instrument will be unable to make accurate measurements.
A sound (vibration) is being emitted by the instrument's jaw.	The jaw may emit sound (vibration) when measuring AC currents in excess of approx. 500 A, however, there is no effect on the measurement.
<ul> <li>The measured value does not appear.</li> <li>No measured value is displayed, even when the test leads are shorted.</li> <li>Zero adjustment is impossible.</li> </ul>	Check the continuity of the test leads. (p.23) If a wiring break is found, replace the test leads.
	Insert the test leads all the way.     Use the proper measurement method.     If no problem can be found, the instrument may be damaged. Send the instrument for repair.

## 4.2 Error display

Error display	Description	Solution
Err 001	ROM error Program	
Err 002	ROM error Adjustment data	When the error appears in the display,
Err 005	ADC error Hardware malfunction	it is necessary to repair the instrument. Please contact your authorized Hioki distributor or reseller.
Err 008	Bluetooth error Hardware malfunction (only for model CM4142)	

#### 4.3 Insert/Replace Batteries

#### **WARNING**

 To avoid electric shock, turn off the instrument and disconnect the test leads before installing or replacing the batteries.




- Handle and dispose of batteries in accordance with local regulations.
- To prevent instrument damage or an electric shock, use only the screw that are originally installed for securing the battery cover in place. If you have lost a screw or find that a screw is damaged, please contact your authorized Hioki distributor or reseller.

The indicator lights up when the battery charge diminishes. Replace the batteries as soon as possible. The batteries may die if the backlight turns on or the buzzer sounds. After use, be sure to turn off the instrument.

#### Insert/Replace Batteries

Screw used to adjust

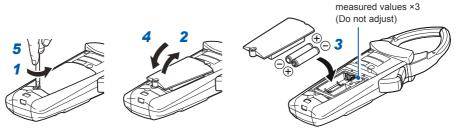

Do not adjust any screws other than the screw holding the battery cover in place. Do not adjust the three screws underneath the cover, which are used to adjust measured values, as doing so may prevent accurate measurement.

Battery indicator	Description
(10)	Fully charged.
(III	As the battery charge diminishes, black charge bars disappear, one by one, from the left of the battery indicator.
<b>_</b>	The battery voltage is low. Replace the batteries as soon as possible.
<u>, , , , , , , , , , , , , , , , , , , </u>	(Flashes) The battery is exhausted. Replace the batteries.

#### 4.4 Cleaning

To clean the instrument, wipe it gently with a soft cloth moistened with water or mild detergent.

## Index

Α	D
AC current       17, 44         AC+DC voltage       17, 52         AC INRUSH       21, 46         AC voltage       17, 47         Auto hold       15, 16         Auto Power Save (APS)       26, 27	DC voltage       17, 27, 5         Diode       17, 24, 5         Disconnection (Breaking)       9, 13, 6         DT4910 Thermocouples (K)       5, 2
AUTO V	Filter
Backlight       26, 27, 62         Bluetooth       11, 29, 61         Breaking (Disconnection)       9, 13, 60         Buzzer sound       22, 27, 62	G GENNECT Cross
C	Jaw 7, 1
Capacitance       24, 57         Continuity       17, 23, 55, 60         Current       14, 33, 38	M           Manual hold         1           MAX value         1

#### Index

Measurement function       11, 17, 22         MIN value       19         Mobile device       11, 29
N
Noise
Ρ
PEAK value
R
Red display       23         Red flash       22         Resistance       17, 23, 56         Rush current       21, 46
s
Serial number 12, 27

# 

#### Z

Zero adjustment	23,	60

Voltage...... 22, 33, 39

# Warranty Certificate

/lodel	Serial number	Warranty period Three (3) years from date of purchase ( / )
Sustomer name: Sustomer address:		
mportant		

# Please retain this warranty certificate. Duplicates cannot be reissued.

address. The personal information you provide on this form will only be used to provide repair service and information Complete the certificate with the model number, serial number, and date of purchase, along with your name and about Hioki products and services.

Please contact the place of purchase in the event of a malfunction and provide this document, in which case Hioki will This document certifies that the product has been inspected and verified to conform to Hioki's standards. repair or replace the product subject to the warranty terms described below.

# Warranty terms

- If the date of purchase is unknown, the warranty period is defined as three (3) years from the date (month and year) of The product is guaranteed to operate properly during the warranty period (three [3] years from the date of purchase). manufacture (as indicated by the first four digits of the serial number in YYMM format).
- If the product came with an AC adapter, the adapter is warrantied for one (1) year from the date of purchase.
- The accuracy of measured values and other data generated by the product is guaranteed as described in the product
- In the event that the product or AC adapter malfunctions during its respective warranty period due to a defect of workmanship or materials, Hioki will repair or replace the product or AC adapter free of charge.
- The following malfunctions and issues are not covered by the warranty and as such are not subject to free repair or replacement:
  - Malfunctions or damage of consumables, parts with a defined service life, etc.
  - 2. Malfunctions or damage of connectors, cables, etc.
- 4. Malfunctions or damage caused by inappropriate handling that violates information found in the instruction manual or Malfunctions or damage caused by shipment, dropping, relocation, etc., after purchase of the product
  - on precautionary labeling on the product itself
    - Malfunctions or damage caused by a failure to perform maintenance or inspections as required by law or recommended in the instruction manual
      - Malfunctions or damage caused by fire, storms or flooding, earthquakes, lightning, power anomalies (involving voltage, frequency, etc.), war or unrest, contamination with radiation, or other acts of God
- -7. Damage that is limited to the product's appearance (cosmetic blemishes, deformation of enclosure shape fading of color, etc.)
- The warranty will be considered invalidated in the following circumstances, in which case Hioki will be unable to perform Other malfunctions or damage for which Hioki is not responsible · ·
  - If the product has been embedded in another piece of equipment for use in a special application (aerospace. -1. If the product has been repaired or modified by a company, entity, or individual other than Hioki service such as repair or calibration:
- If you experience a loss caused by use of the product and Hioki determines that it is responsible for the underlying issue, nuclear power, medical use, vehicle control, etc.) without Hioki's having received prior notice
- Secondary damage arising from damage to a measured device or component that was caused by use of the product Hioki wi∎ provide compensation in an amount not to exceed the purchase price, with the following exceptions:
  - Damage arising from measurement results provided by the product
- Damage to a device other than the product that was sustained when connecting the device to the product (including via network connections)
- 8. Hioki reserves the right to decline to perform repair, calibration, or other service for products for which a certain amount of time has passed since their manufacture, products whose parts have been discontinued, and products that cannot be repaired due to unforeseen circumstances.

HIOKI E.E. CORPORATION http://www.hioki.com

# HIOKI



All regional contact information

#### http://www.hioki.com

#### **HEADQUARTERS**

81 Koizumi Ueda, Nagano 386-1192 Japan

#### **HIOKI EUROPE GmbH**

Rudolf-Diesel-Strasse 5 65760 Eschborn, Germany hioki@hioki.eu

1906 EN

Edited and published by HIOKI E.E. CORPORATION

Printed in Japan

- •CE declarations of conformity can be downloaded from our website.
- ·Contents subject to change without notice.
- This document contains copyrighted content.
- It is prohibited to copy, reproduce, or modify the content of this document without permission.
- Company names, product names, etc. mentioned in this document are trademarks or registered trademarks of their respective companies.

HIOKI CM4141A961-03